



1 / 6

FIG. 1

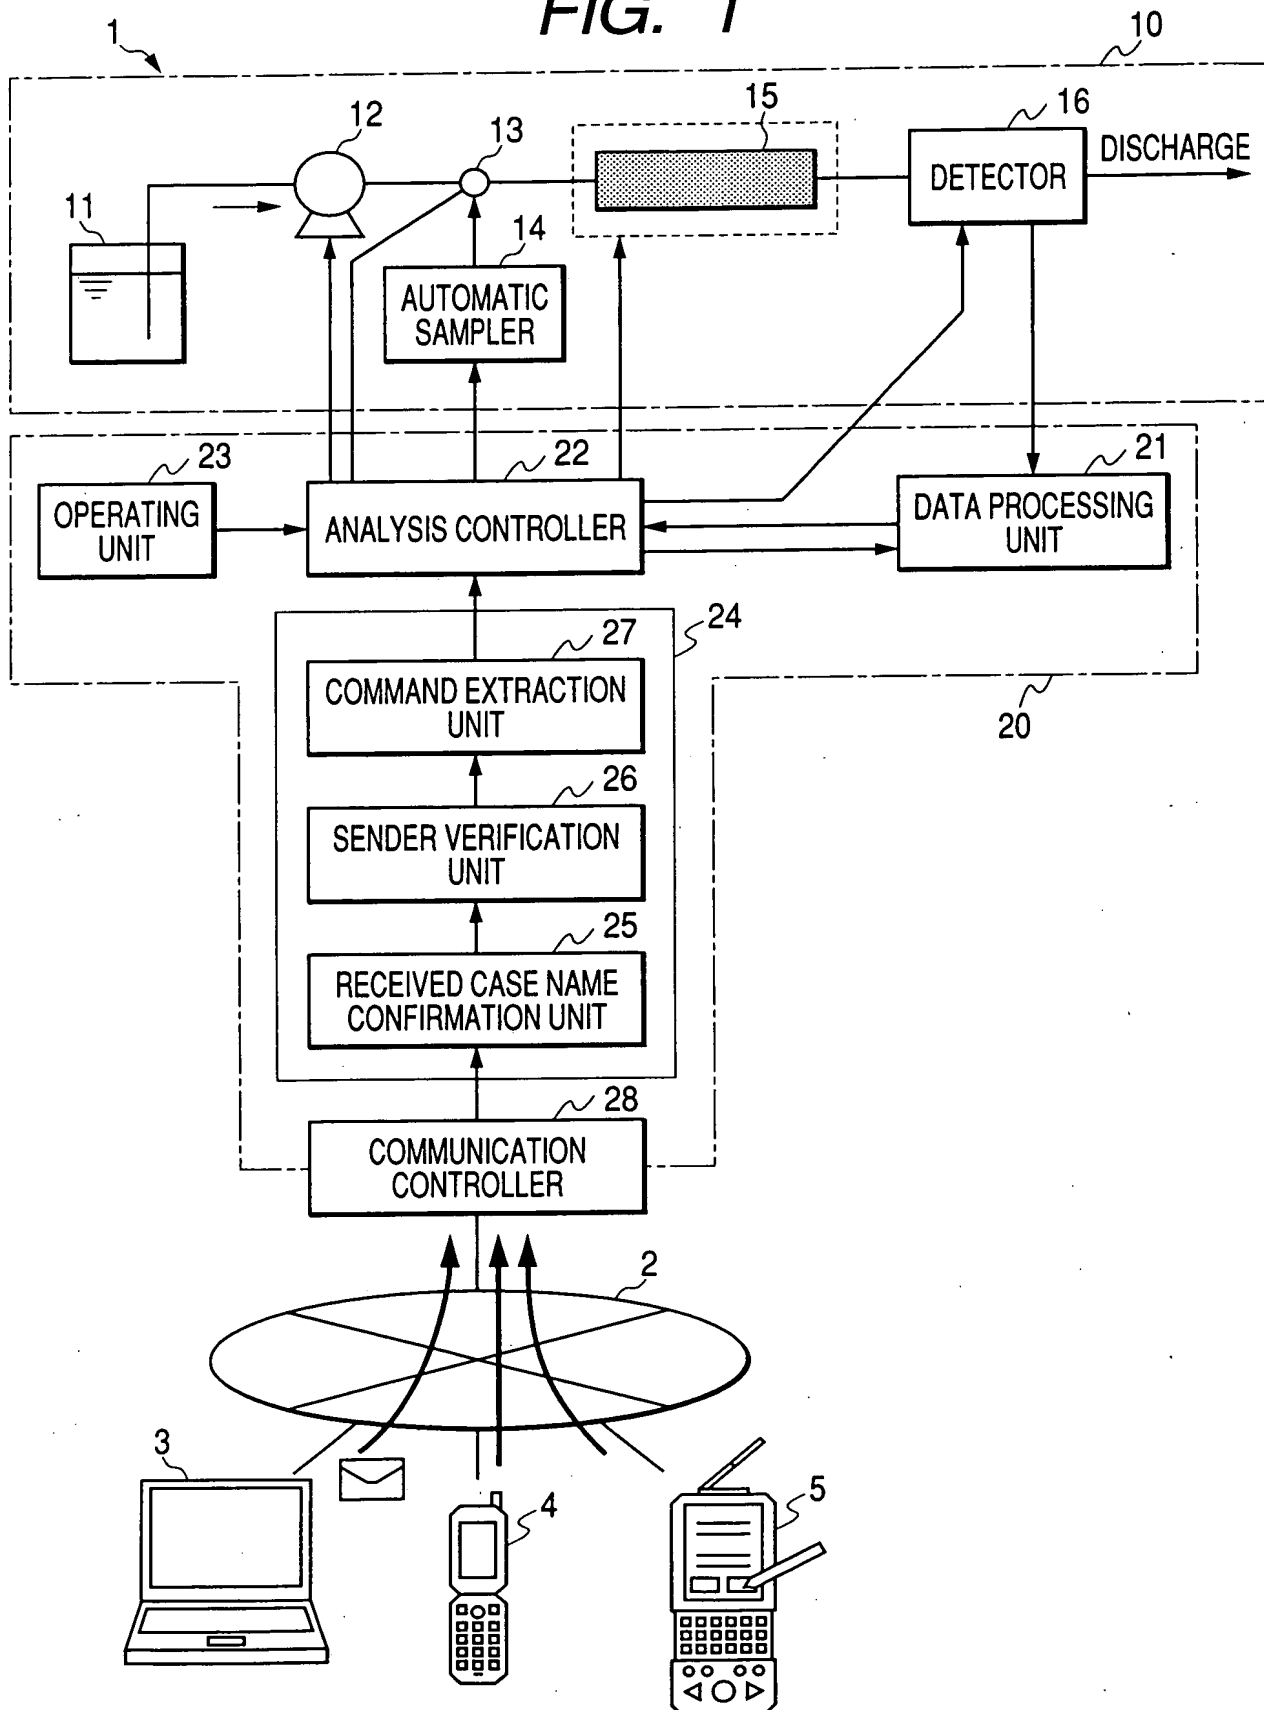


2 / 6

FIG. 2

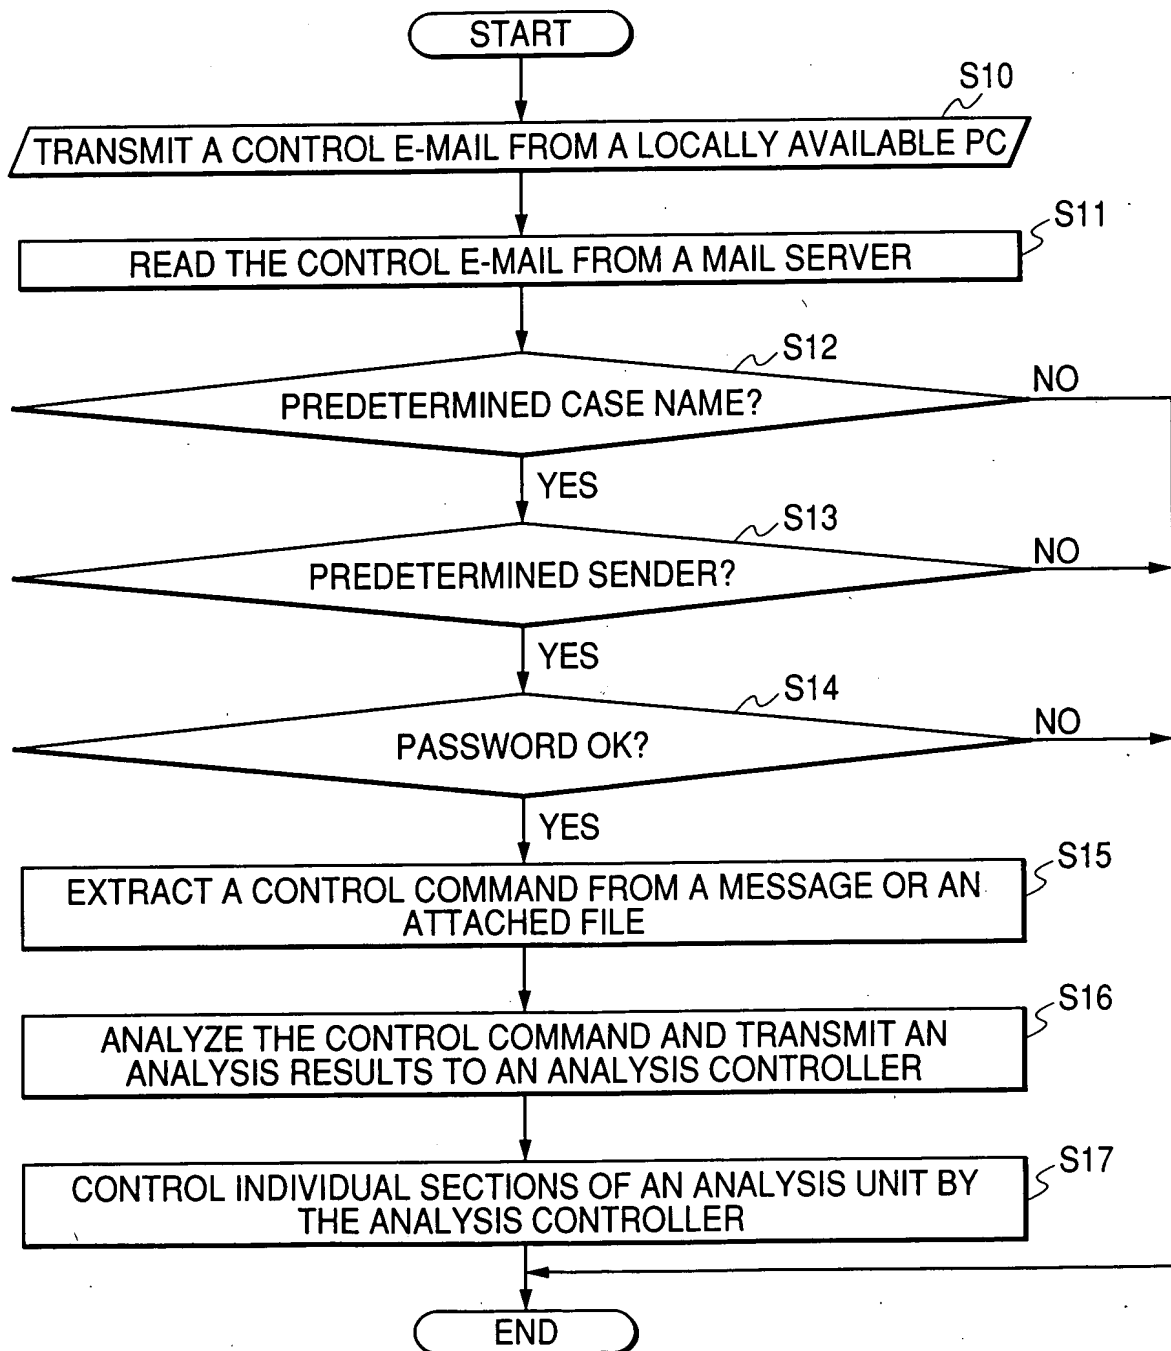

3 / 6

FIG. 3

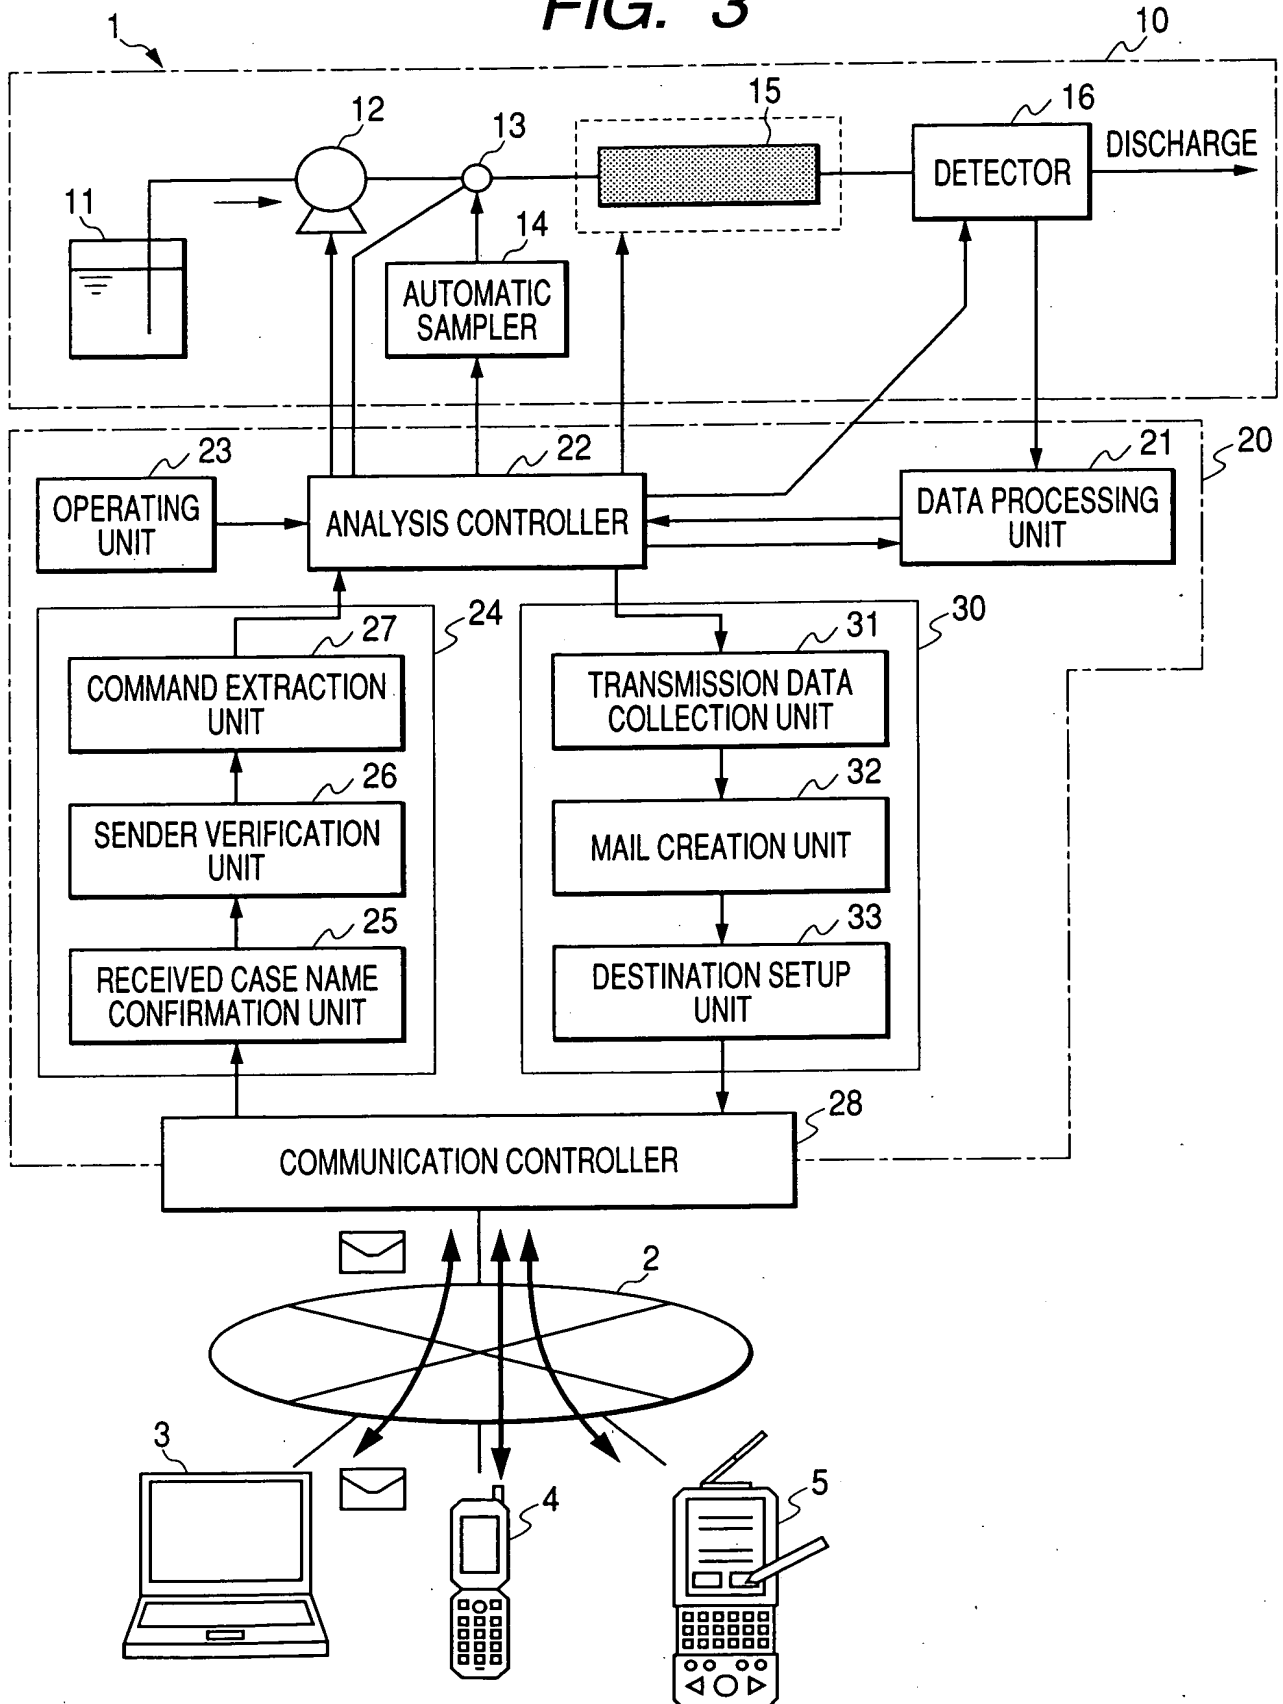

4 / 6

FIG. 4

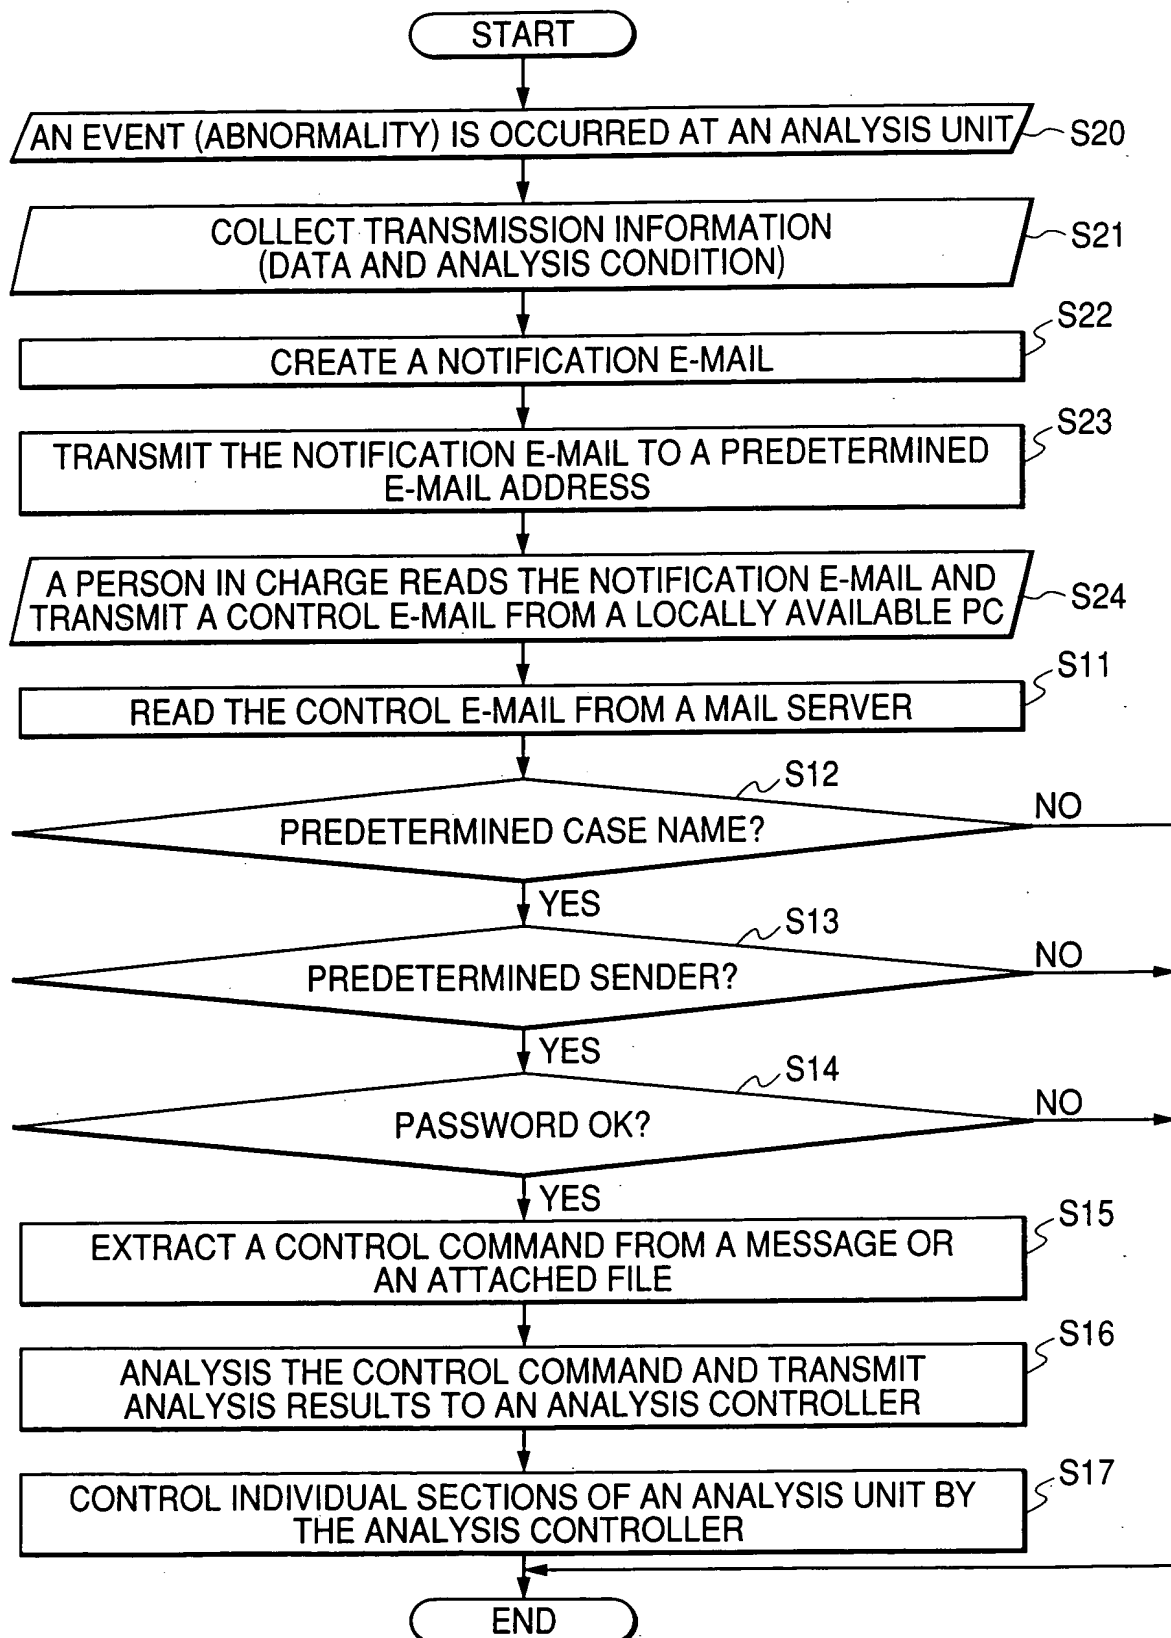


FIG. 5

TRANSMISSION SERVER : LC#1
 TRANSMISSION DATE AND TIME : 19:58, AUGUST 2, 2002
 DESTINATION : ○○○○
 CASE NAME : REPORT OF STATUS OF AUTOMATIC ANALYSIS LC#1

SINCE RESULTS OF THE FOLLOWING REPRODUCTION TEST SHARED A DISQUALIFICATION,
 THE ANALYSIS OPERATION WAS HALTED.

DATE AND TIME 2002/8/2 19:55
 CATEGORY RETENTION TIME
 THE NUMBER OF DATA SETS USED 7
 THE NUMBER OF IDENTICAL PEAKS 5

INDIVIDUAL PEAK	CV VALUES	1.3%	0.8%	8.1%(DISQUALIFIED)	1.7%	2.2%
PEAK 1 DATA	1.11	1.13	1.14	1.15	1.15	1.15
PEAK 2 DATA	1.72	1.71	1.71	1.75	1.72	1.71
PEAK 3 DATA	2.30	2.50	2.90	2.50	2.50	2.30
PEAK 4 DATA	3.10	3.00	3.00	3.00	3.10	3.10
PEAK 5 DATA	4.50	4.50	4.55	4.57	4.55	4.80

DO YOU WANT TO RESUME THE ANALYSIS OPERATION?

A : RESUME ANALYSIS
 B : PERFORM ANALYSIS AGAIN FROM THE BEGINNING, AFTER AN ANALYSIS CONDITION IS STABILIZED.
 → PLEASE DESIGNATE AN ANALYSIS CONDITION SETUP FILE.

- 1 : RINSE A COLUMN (ORGANIC SOLVENT)
- 2 : RINSE A COLUMN (ACID SOLVENT)
- 3 : REMOVE BUBBLES
- 4 : PREPROCESS A
- 5 : PREPROCESS B
- 99: ATTACH A METHOD FILE (PLEASE ATTACH A FILE)
- C : TRANSMIT AN ANALYSIS CONDITION

6 / 6

FIG. 6

	A	B	C	D	E	F	△
2							
3		METHOD FILE NAME	METHOD1				
4							
5		ANALYSIS CONDITION					
6							
7		FLOW RATE OF LIQUID	A	0.2	μ L/min		
8	B		0.2	μ L/min			
9	C		0	μ L/min			
10		UPPER PRESSURE LIMIT VALUE	A	10	MPa		
11	B		0	MPa			
12	C		0	MPa			
13							
14		COLUMN TEMPERATURE		40	°C		
15			UPPER LIMIT VALUE	65	°C		
16							
17		DETECTOR A	ANALYSIS PERIOD	5	min		
18			WAVELENGTH	245	nm		
19			SAMPLING RATE	100	msec		
20							
21		DETECTOR B	ANALYSIS PERIOD	5	min		
22			WAVELENGTH	245	nm		
23			SAMPLING RATE	100	msec		
24							
25		PEAK DETECTION	WIDTH	1	sec		
26			SLOPE	10000	μ V/sec		
27			DRIFT	1000	μ V/hour		
▽							
◀ ▶ ▷ ◂ ▸ \ METHOD / DETERMINATION METHOD / ◀ ▶							